



TEST REPORT TUCHENG

Date: Aug. 28, 2020 **Date of Receipt:** Jul. 31, 2020
Report No.: TAG9G842-C **Quantity:** 1PC **Page Order/Pages:** (P1/2) **Ref. No.:** NIL
Report Title: Art Beauty Group Company Limited(HK172) **Item:** Mask
Address: Unit 2305, Apec Plaza, 49 Hoi Yuen Road, Kwun Tong, Kowloon

Test Items		Test Results	Test Methods
Bacterial Filtration	1	99.8	CNS 14775 T4037-2003
Efficiency (BFE)(%)	2	99.7	
Staphylococcus aureus	3	99.7	
ATCC 6538	4	99.8	
	5	99.6	

Note: Control average: 2675 CFU.

Note: Mean particle size: 3.0 μm.


Note: Testing side: outside of specimen.

Note: Testing area: 39.5 cm².

Note: Flow rate: 28.3 L/min.

Note: Sample description is given by the client: Surgical face mask

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

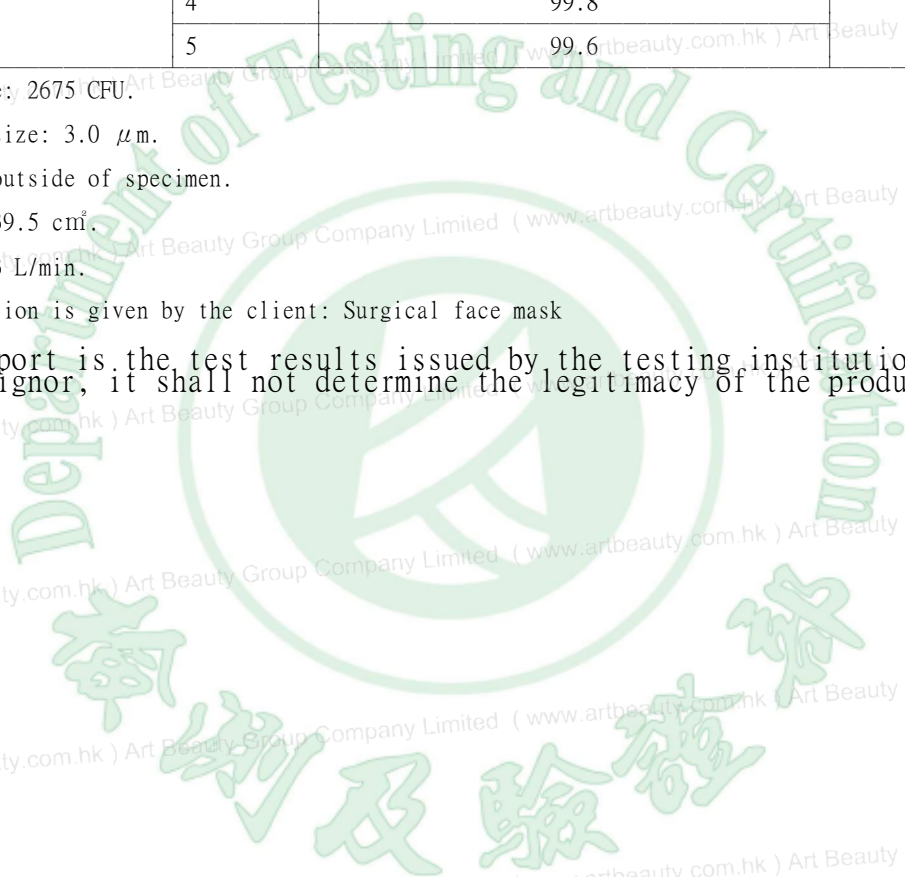

Note: 1. This report is only responsible for the submitted sample(s), which will be kept for one month period.

2. This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3. The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung Kao
Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108, +886-2-22689839



TEST REPORT TUCHENG


Date: Aug. 28, 2020 **Date of Receipt:** Jul. 31, 2020
Report No.: TAG9G842-B **Quantity:** 1PC **Page Order/Pages:** (P1/2) **Ref. No.:** NIL
Report Title: Art Beauty Group Company Limited(HK172) **Item:** Mask
Address: Unit 2305, Apec Plaza, 49 Hoi Yuen Road, Kwun Tong, Kowloon

Test Items		Test Results	Test Methods
Air Exchange Pressure (mmH2O/cm ²)	1	2.7	CNS 14774 T5017-2018 9.4
	2	2.7	CNS 14777 T4039-2003
	3	2.7	
	4	2.5	
	5	2.7	

Note: Air Exchange Pressure takes 5 masks for testing.

Note: Sample description is given by the client: Surgical face mask

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

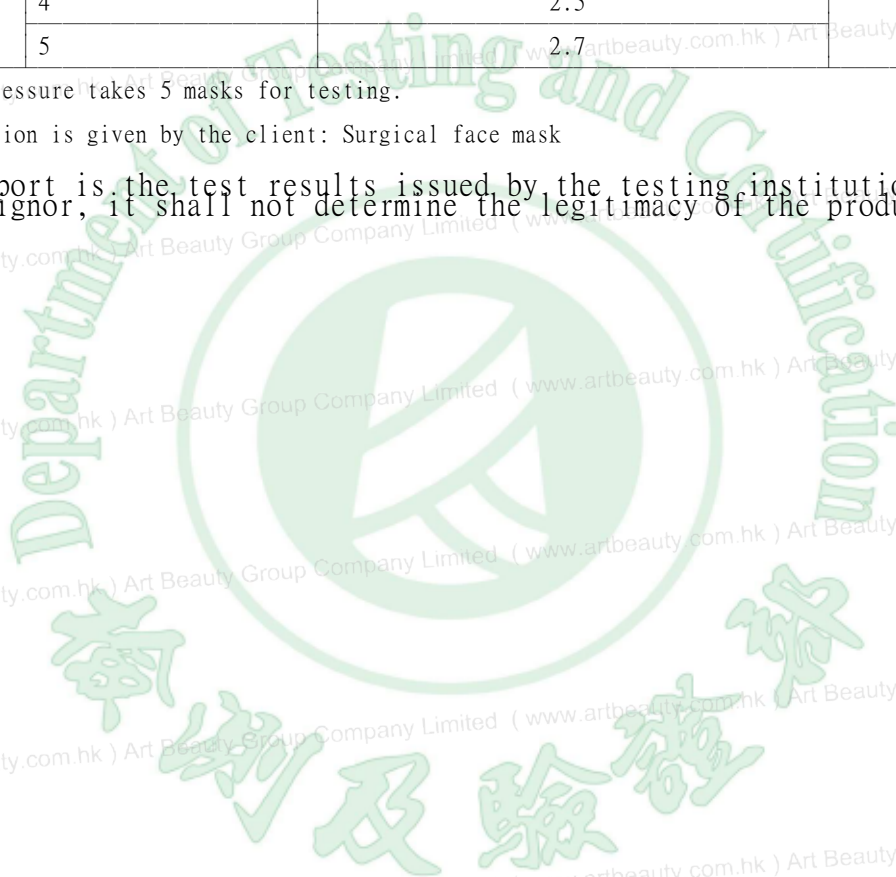

Note: 1. This report is only responsible for the submitted sample(s), which will be kept for one month period.

2. This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3. The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung Kao
Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108, +886-2-22689839




TEST REPORT TUCHENG

Date: Aug. 28, 2020 **Date of Receipt:** Jul. 31, 2020
Report No.: TAG9G842-A **Quantity:** 1PC **Page Order/Pages:** (P1/2) **Ref. No.:** NIL
Report Title: Art Beauty Group Company Limited(HK172) **Item:** Mask
Address: Unit 2305, Apec Plaza, 49 Hoi Yuen Road, Kwun Tong, Kowloon

Test Items	Test Results		Test Methods
	Pressure: 80 mmHg	Pressure: 120 mmHg	
Synthetic Blood Penetration	1	None Seen	CNS 14774 T5017-2018 9.1
	2	None Seen	CNS 14776 T4038-2003
	3	None Seen	
	4	None Seen	
	5	None Seen	
	6	None Seen	
	7	None Seen	
	8	None Seen	
	9	None Seen	
	10	None Seen	
	11	None Seen	
	12	None Seen	
	13	None Seen	

Note: Sample description is given by the client: Surgical face mask

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

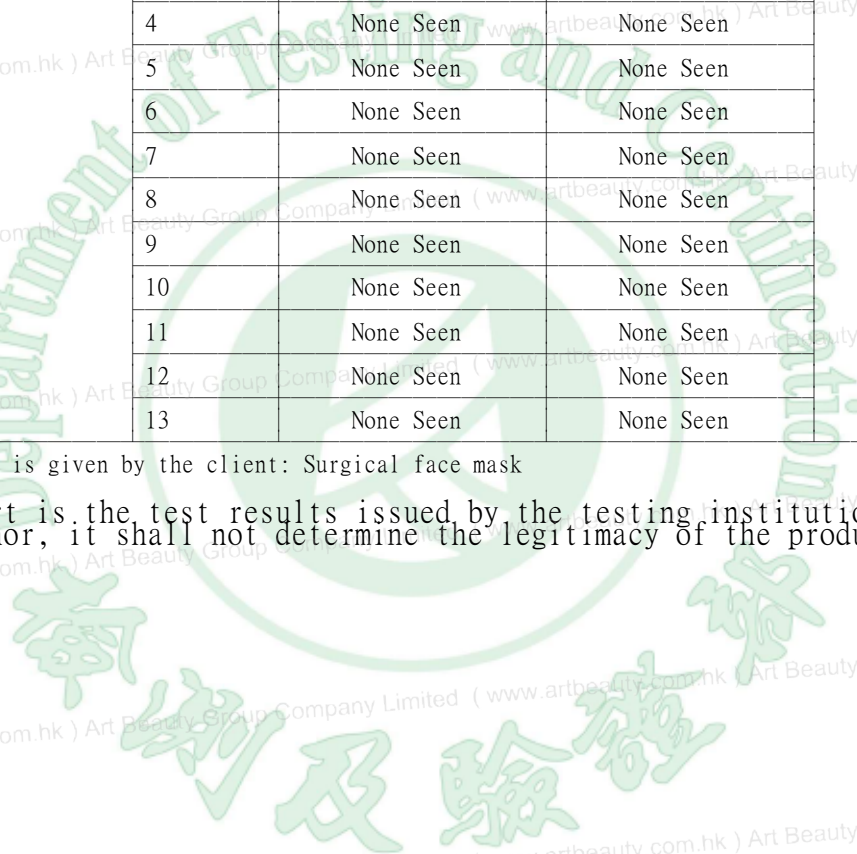

- Note:**
- This report is only responsible for the submitted sample(s), which will be kept for one month period.
 - This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
 - The test report should not be used for public advertisement and commercial promotion.

Authorized by president of
Taiwan Textile Research Institute

Jui-hung kao
Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
 No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
 Tel : +886-2-22670321 ext. 7107, 7110
 Fax : +886-2-22675108, +886-2-22689839